


Figure 1
 Van Ness Station
 AM Peak Period Volume-to-Capacity Ratio for Key Station Elements

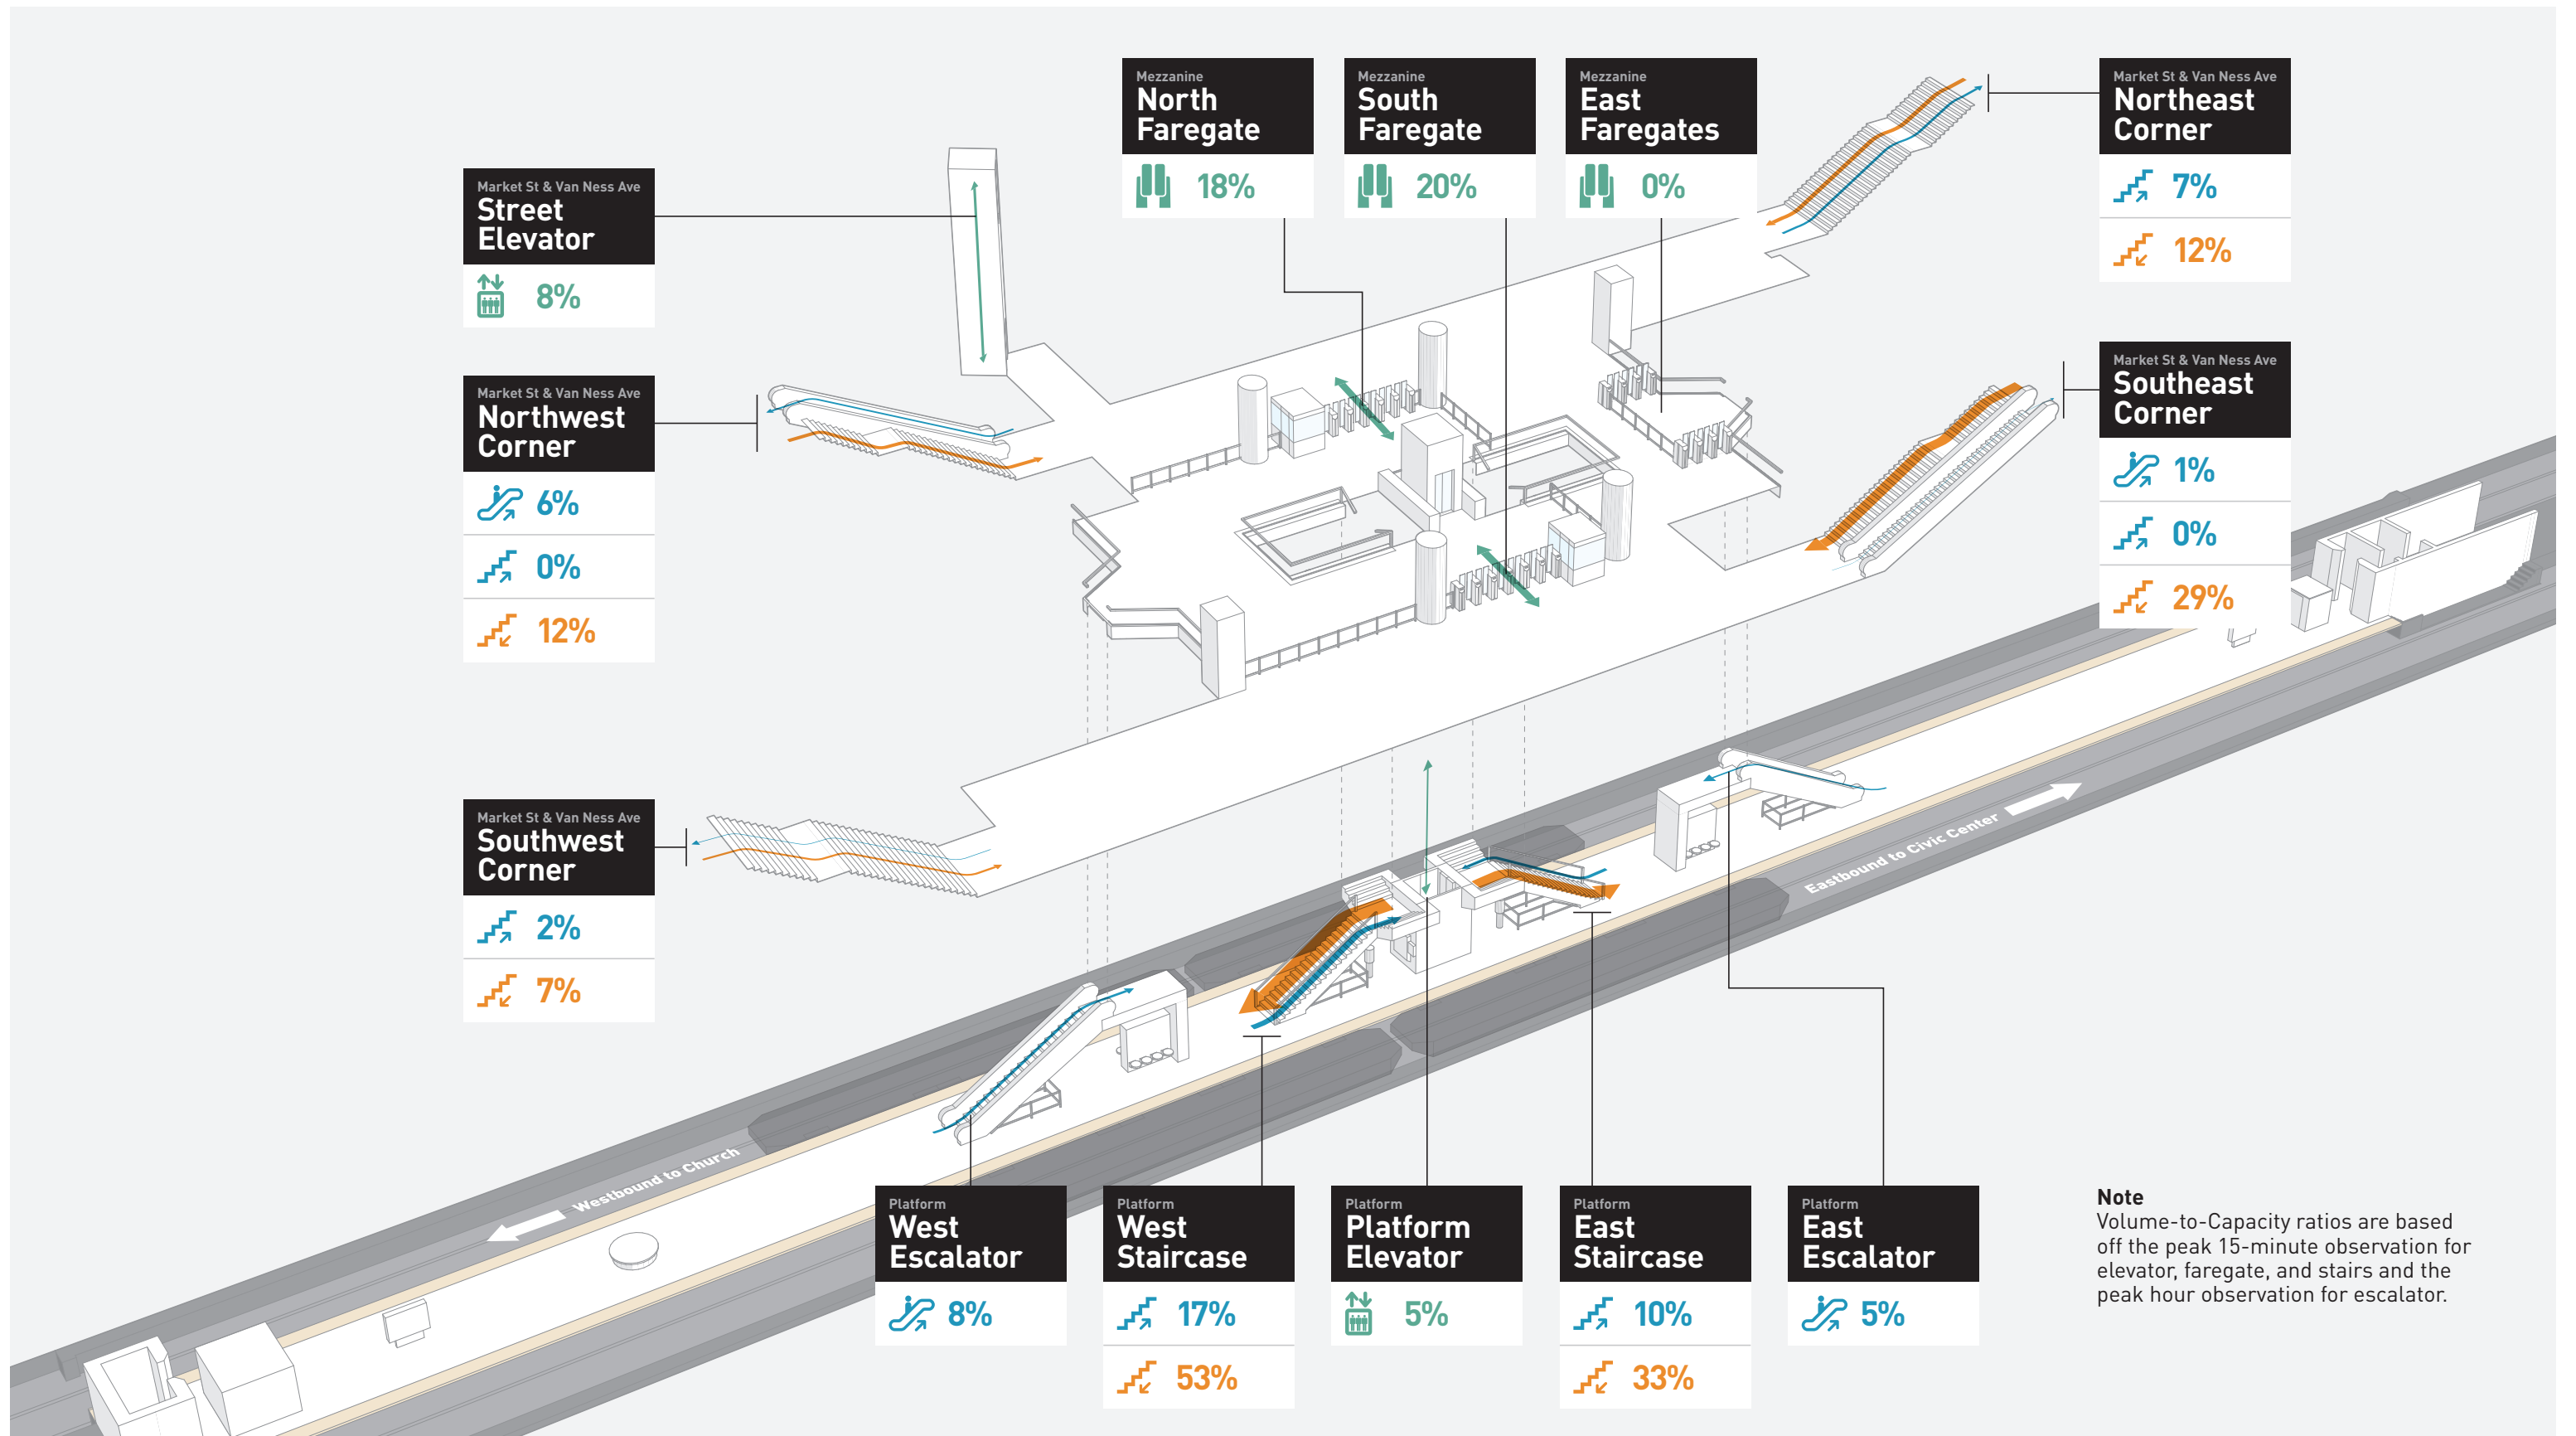

Note
 Volume-to-Capacity ratios are based off the peak 15-minute observation for elevator, faregate, and stairs and the peak hour observation for escalator.



Figure 2
 Van Ness Station
 PM Peak Period Volume-to-Capacity Ratio for Key Station Elements

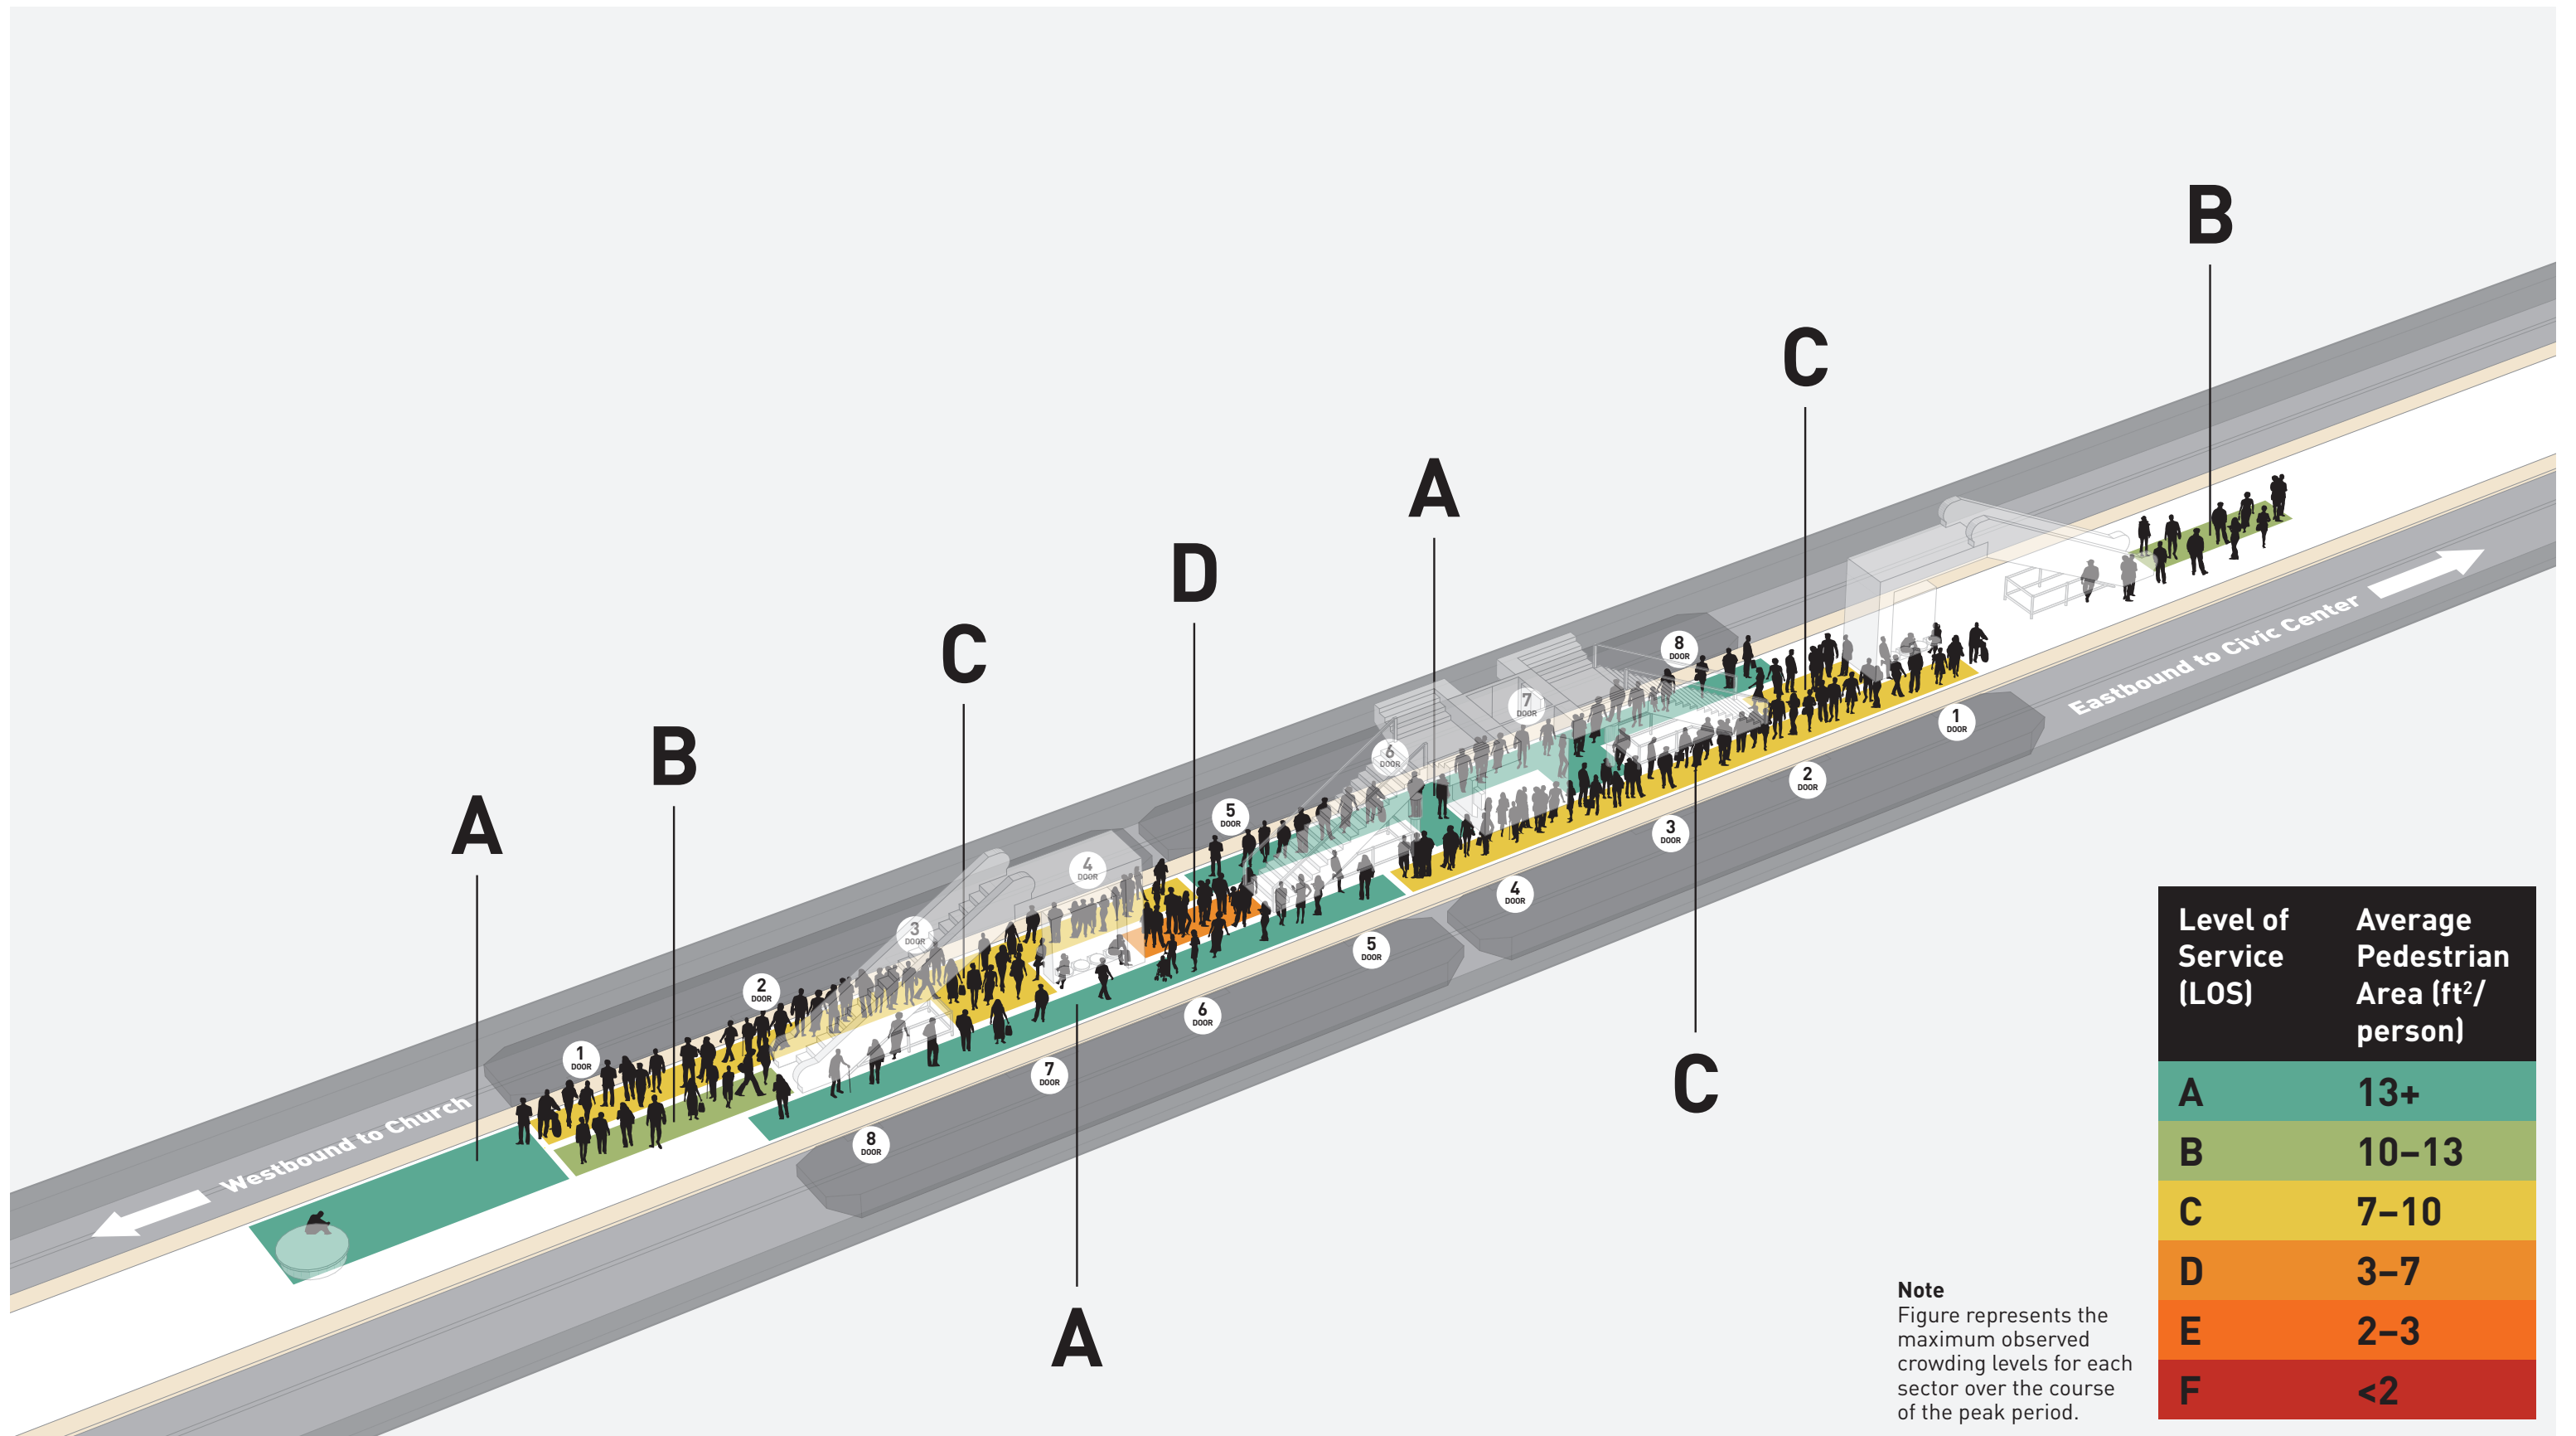


Figure 3
Van Ness Station
AM Peak Period Platform Crowding

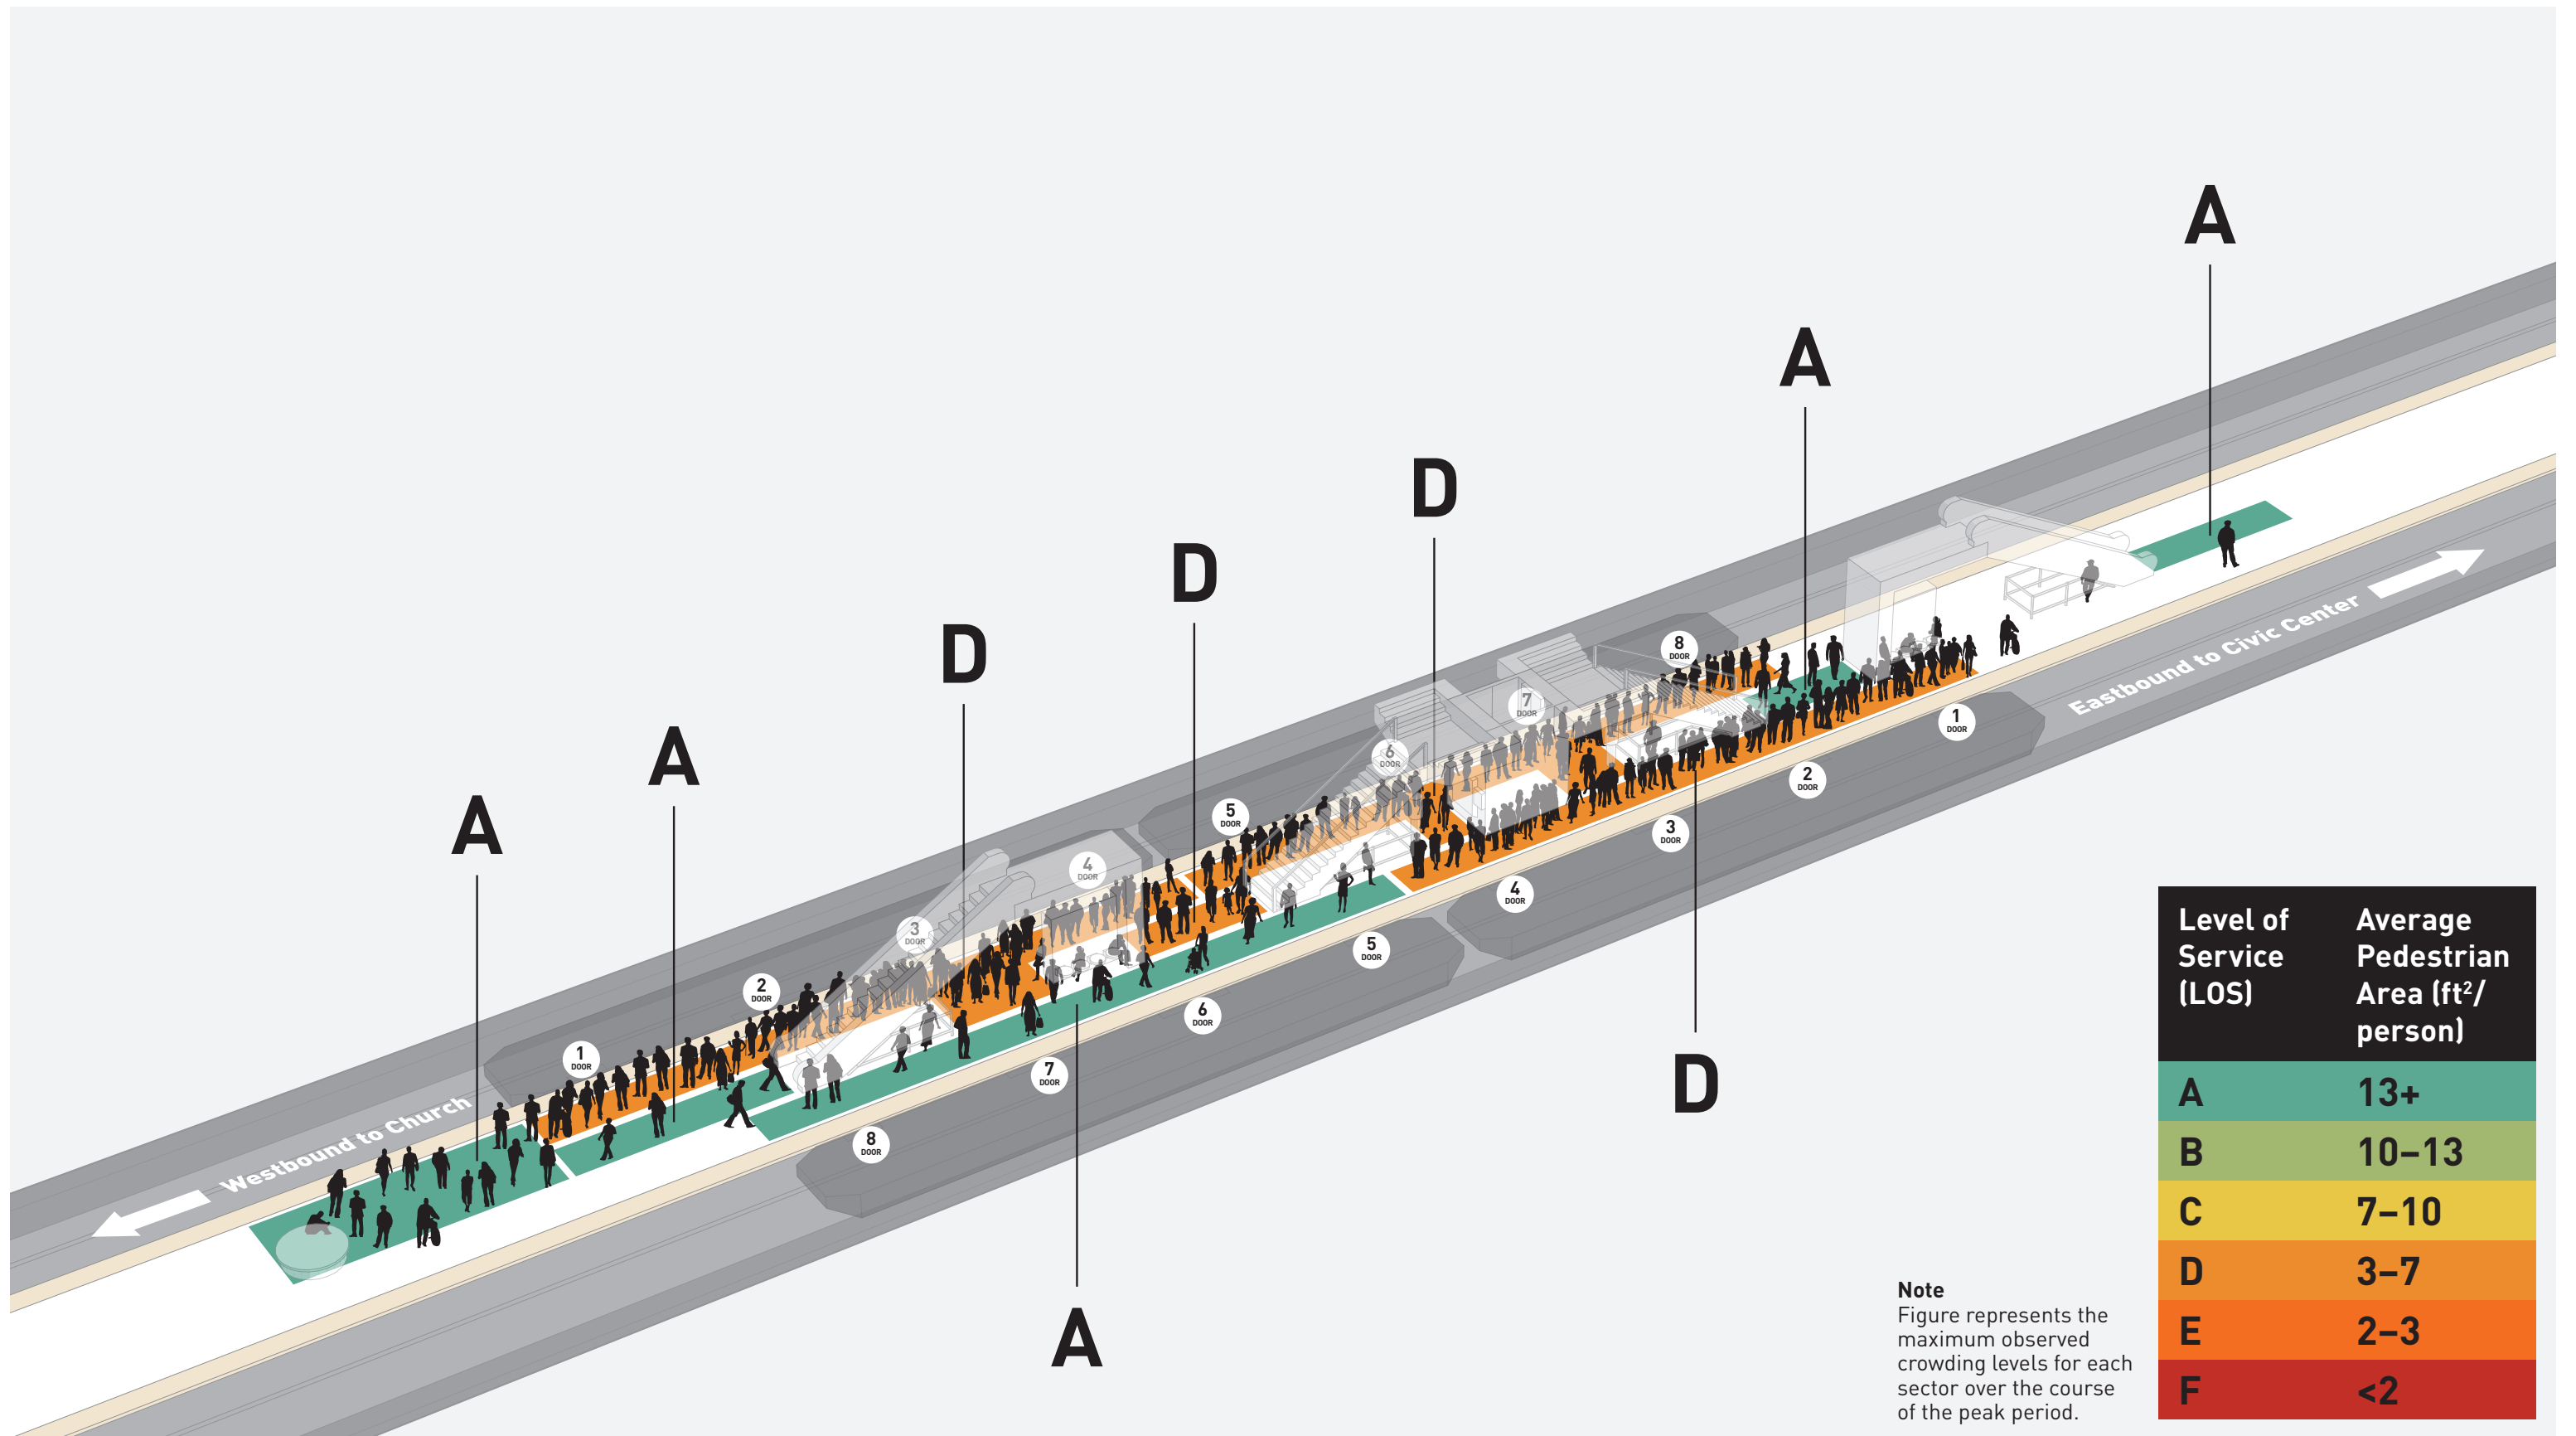


Figure 4
Van Ness Station
PM Peak Period Platform Crowding